

Manufacturer: MIKROTREND d.o.o. 4.Bizek 14, 10000 Zagreb, CROATIA
e-mail: info(at)mikrotrend.com www.mikrotrend.com

Date: 24. April 2013

Ambient: 26°C

Test performed by: K. Pavlovic

Manufacturers test and calibration report no:

Sample

Product name: **Air Gap Sensor**
with:

Part No.: **AGSP-25**

Ser. No.: **S-Sample**


Product name: **Air Gap Conditioner**

Part No.: **AGSC-25**

Ser. No.: **C-Sample**

Scope of testing: **tested and recorded sensor output at specified distance from sensors surface**

Distance	Output voltage	Output voltage	Test result
d(mm)	Videal(V)	Vmeasured(V)	Error(%)
4,7	1,88	1,88	0,00
6,7	2,68	2,61	-2,61
8,7	3,48	3,38	-2,87
10,7	4,28	4,2	-1,87
12,7	5,08	5,03	-0,98
14,7	5,88	5,88	0,00
16,7	6,68	6,72	0,60
18,7	7,48	7,55	0,94
20,7	8,28	8,36	0,97
22,7	9,08	9,15	0,77
24,7	9,88	9,88	0,00

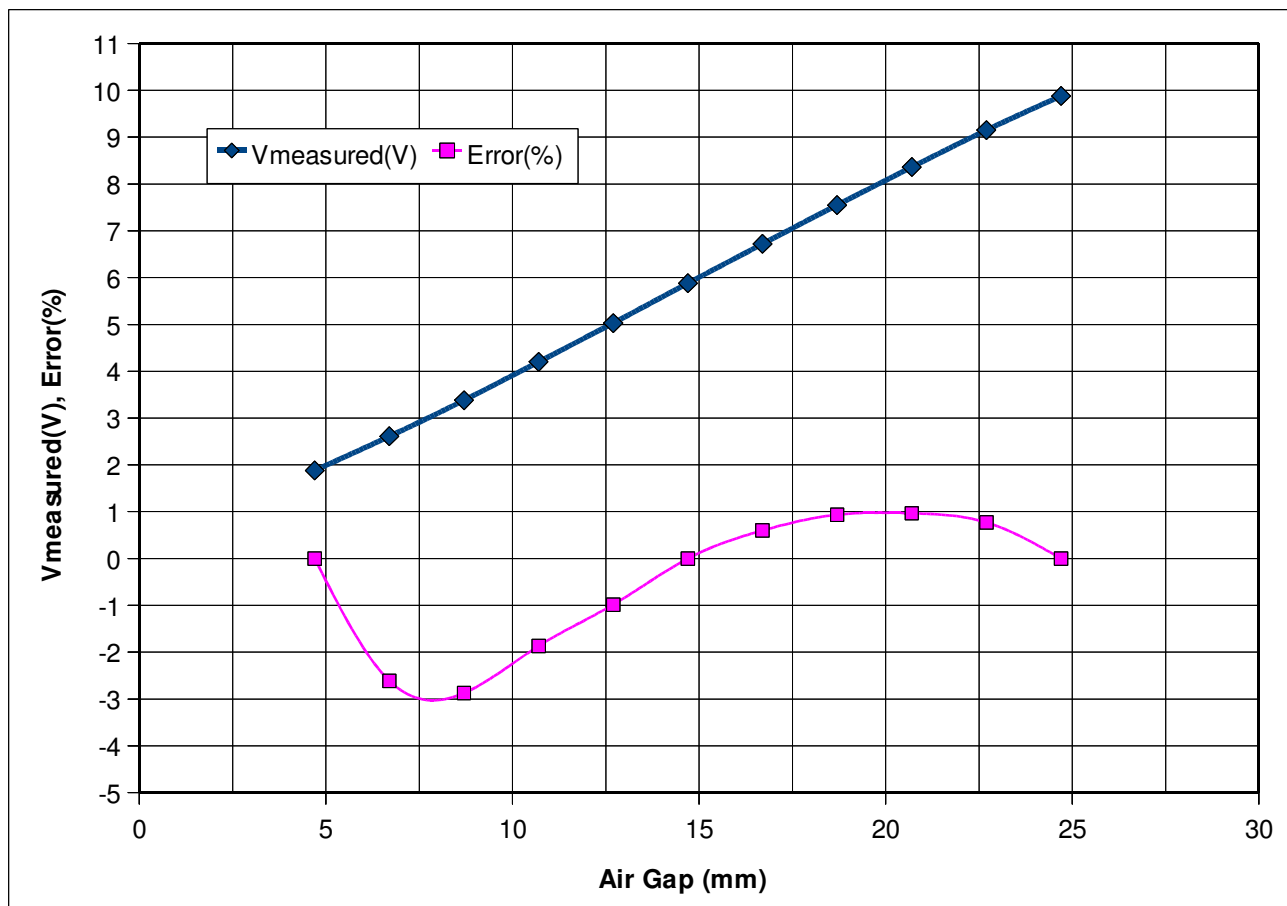

The product and the factory surveillance system meet all applicable requirements as laid down in the relevant Installation and user manual